



The potential of fiber-optic probe for soluble solid content prediction, in intact sugar beet

R. Bendoula, Alexia Gobrecht, Arnaud Ducanhez, A. Herrero, P. Guerrero
Castroa, J.M. Roger

► To cite this version:

R. Bendoula, Alexia Gobrecht, Arnaud Ducanhez, A. Herrero, P. Guerrero Castroa, et al.. The potential of fiber-optic probe for soluble solid content prediction, in intact sugar beet. 17th International Conference on Near Infrared Spectroscopy, Oct 2015, Foz do Iguassu, Brazil. pp.1, 2015. hal-02602089

HAL Id: hal-02602089

<https://hal.inrae.fr/hal-02602089>

Submitted on 16 May 2020

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

The potential of fiber-optic probe for soluble solid content prediction, in intact sugar beet



R. Bendoula, A. Gobrecht, A. Ducanchez, A. Herrero, P. Guerrero-Castroa, J. M. Roger

IRSTEA, UMR ITAP, 361 rue JF Breton, 34196 Montpellier, France




Context

Sugar beet is the second biggest world contributor to sugar production and the only one grown in Europe. One of the main limitations for its competitiveness is the lack of effective tools for assessing sugar content in unprocessed sugar beet roots, specially in breeding programs. In this context, a dedicated NIR fiber-optic probe is proposed as a suitable approach. NIR technology is widely used for the estimation of sugar content in vegetable products, while optic fibers allow a wide choice of technical properties and configurations that can be specifically adapted as needed.

The objective of this work is to evaluate the effect of probe design (single fiber probe (SFP) and multiple fiber probe (MFP)) for the estimation of Soluble Solid Content (SSC) in intact sugar beets.

Comparison is made based on the analysis of the measured spectra and the performance of the calibration models. In addition, the impact of different optical components of the probe were analyzed, such as fiber diameter, distance between illumination and collection fiber in order to optimize the optical setup of the probe.

Materials and methods

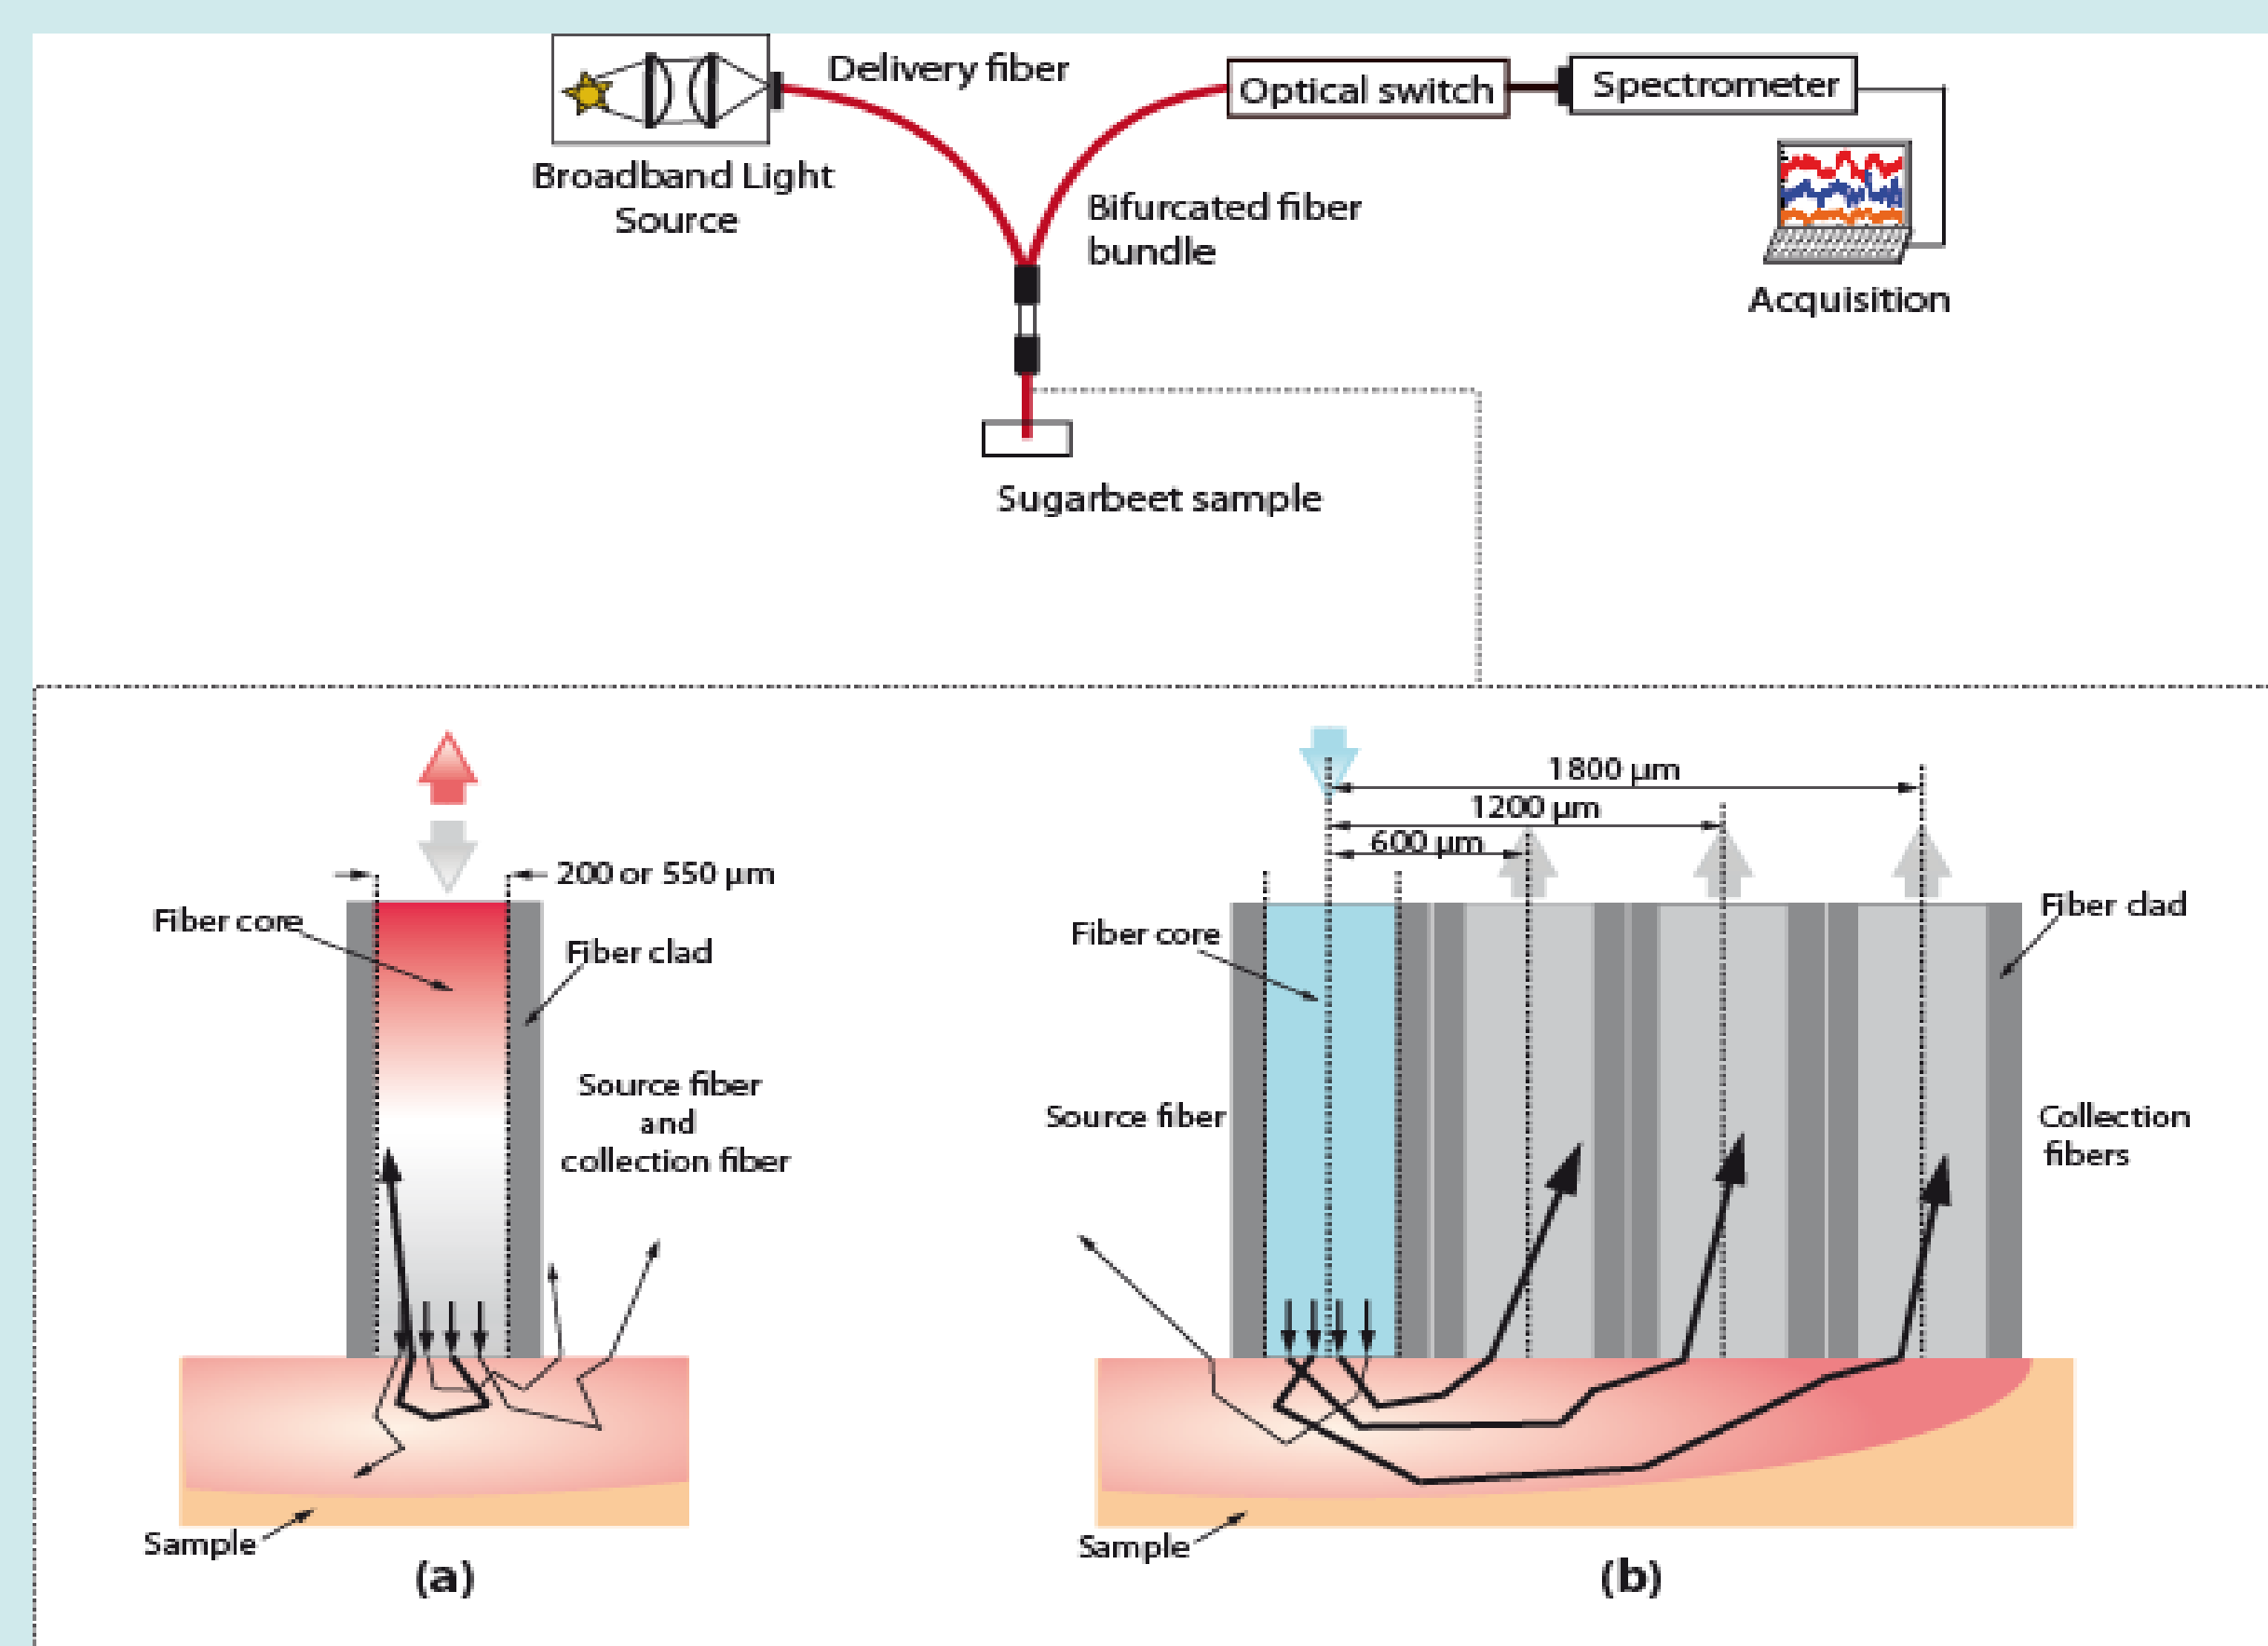

Optical configurations	Number of beet samples	Mean sucrose value (brix)	Standard deviation (brix)	Sucrose content range (brix)
Single-fiber probe D= 200μm	170	24,31	6,49	[17,8 – 45,2]
Single-fiber probe D= 550μm	170	24,67	6,96	[17,1 – 43,2]
Mutiple-fiber probes (all positions)	170	24,42	6,65	[17,1 – 45,5]

Table : Soluble solid content values for the different batch per optical configuration

Figure: a) Schematic diagram of the single- fiber probe. b) schematic diagram of the multiple-fiber probes (F1 at 600 μm, F2 at 1200 μm and F3 at 1800 μm).

Results

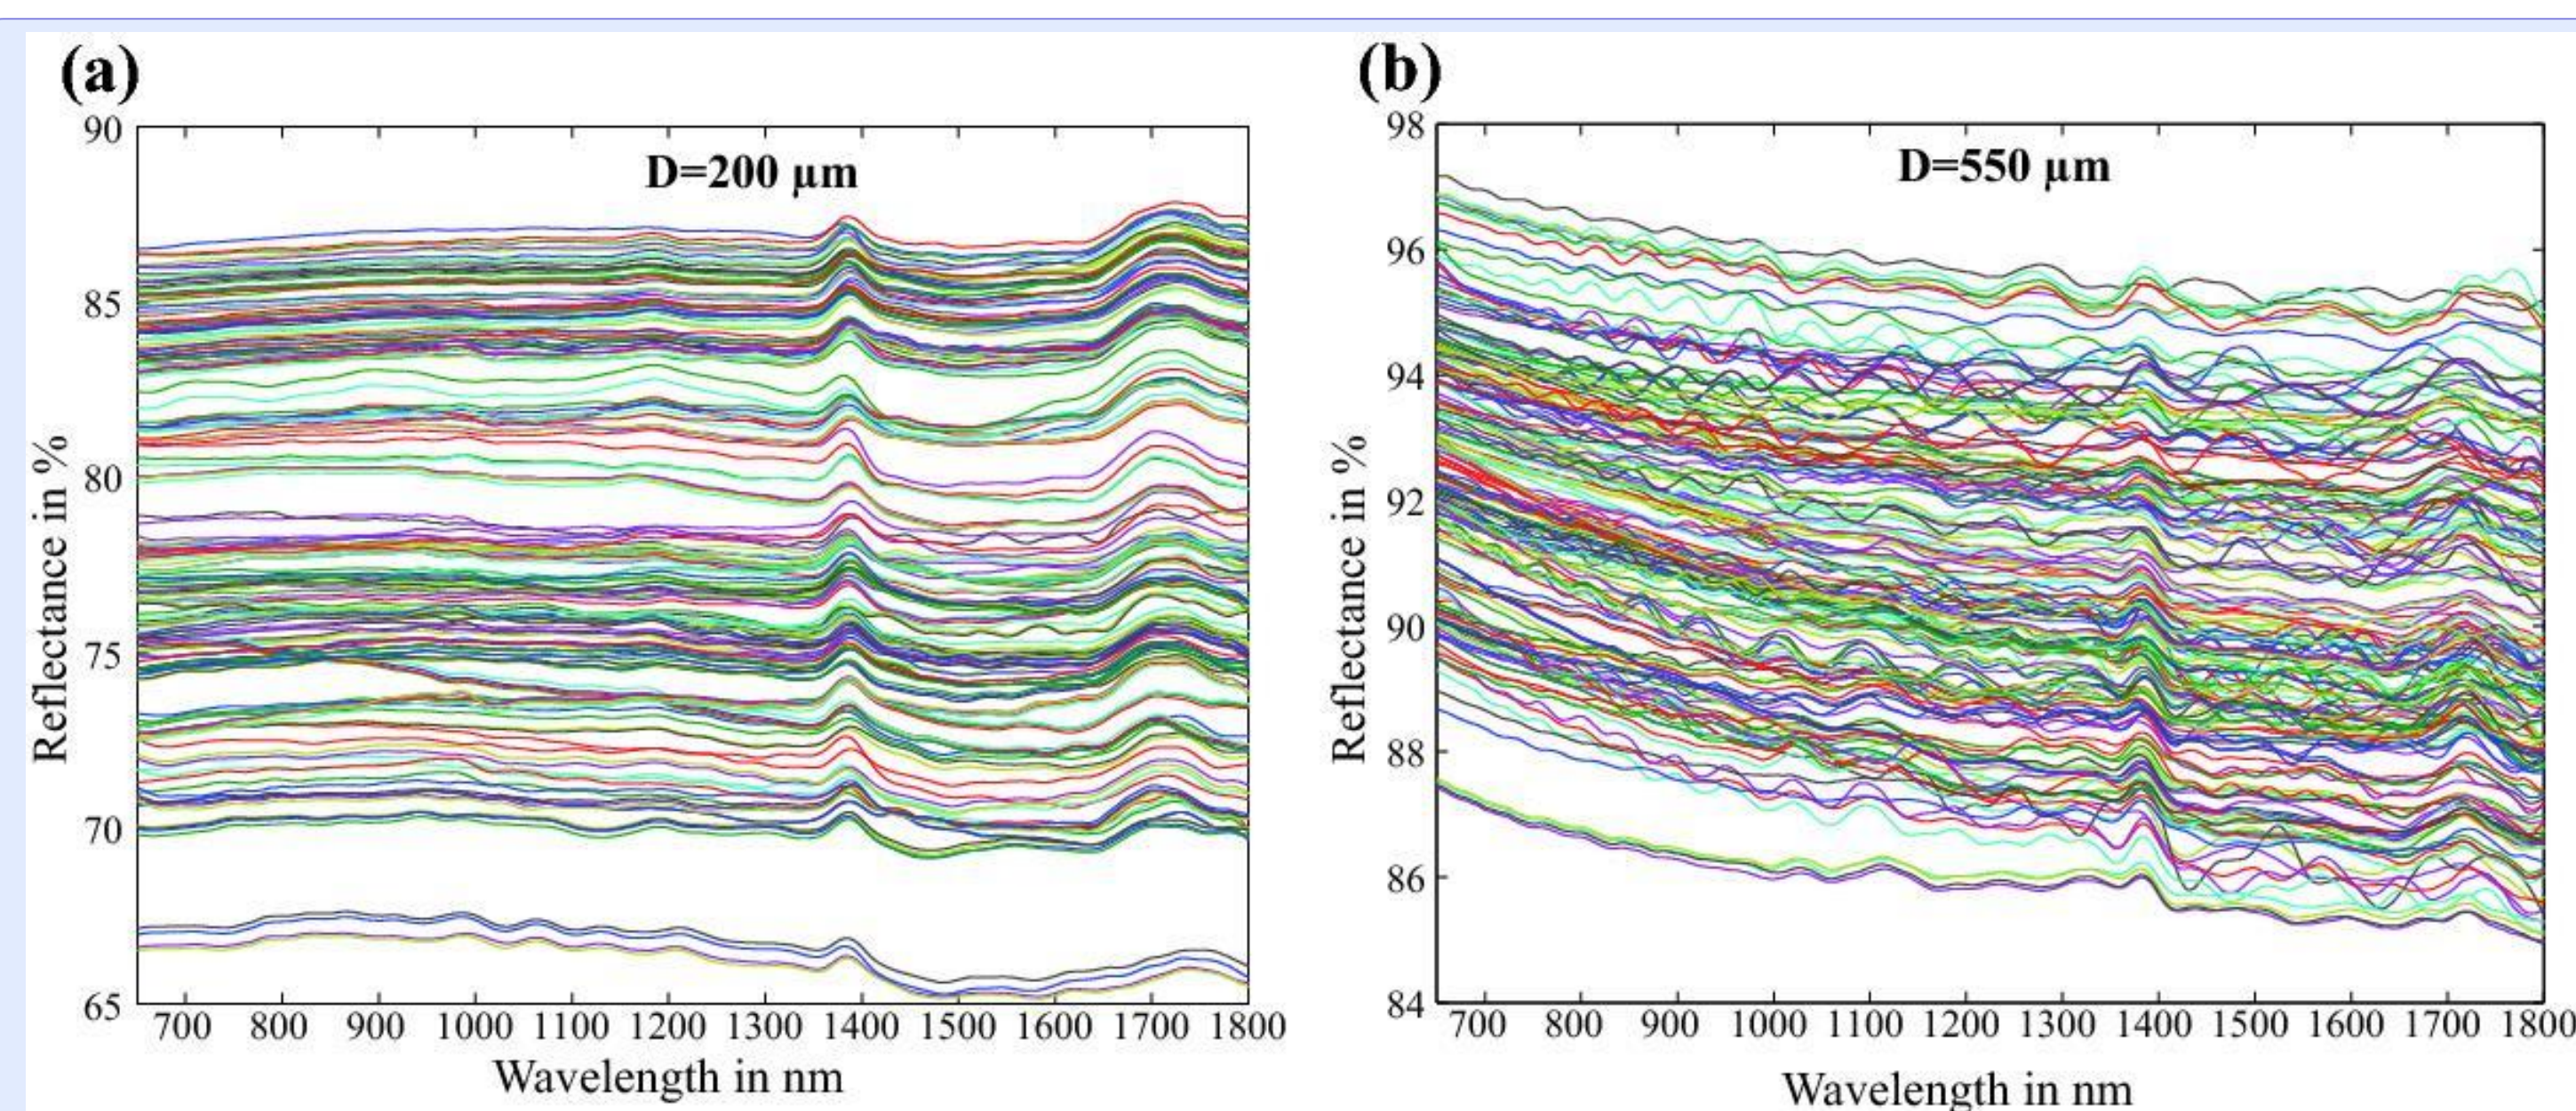


Figure : Raw reflectance spectra of the single-fiber probe with two diameter (a) 200 μm. (b) 550 μm .

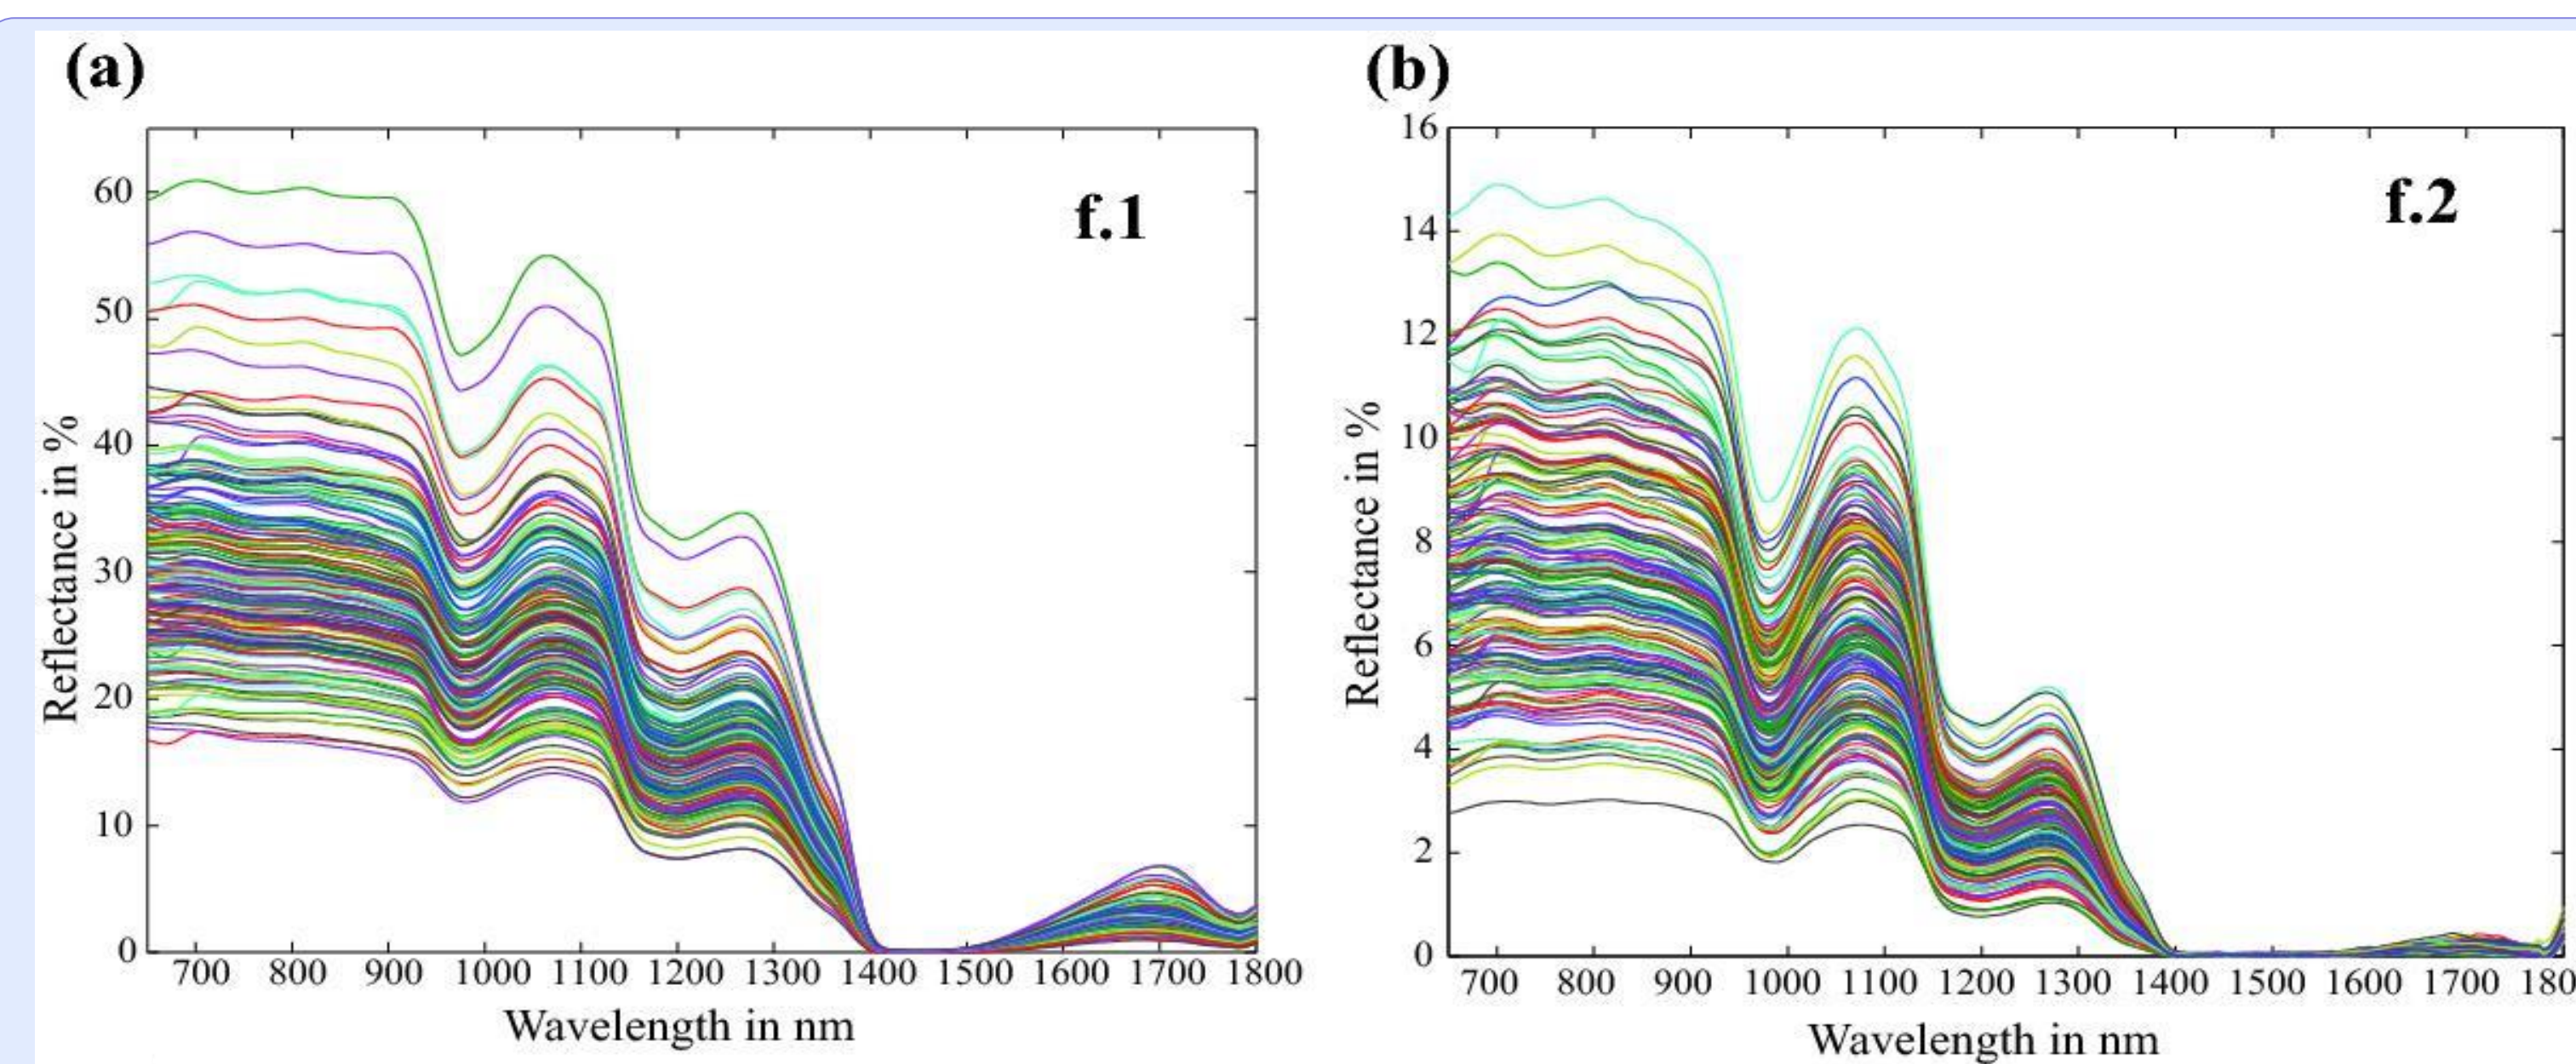


Figure: Raw reflectance of the multiple-fiber probes (a) position F1 of the collecting fiber (b) position F2 of the collecting fiber.

Optical configuration	Preprocessing	R^2_c	SEC (brix)	R^2_p	SEP _c (brix)	RPD
Single fiber probe D=200μm	SG1	0,69	3,66	0,757	3,21	2,02
Single fiber probe D=550μm	SG1	0,645	3,93	0,689	3,95	1,76
Multiple fiber probe F1	SNV	0,95	1,49	0,904	1,95	3,36
Multiple fiber probe F2	SNV	0,927	1,81	0,908	1,94	3,38
Multiple fiber probe F3	SNV	0,828	2,75	0,807	2,8	2,347

Table : Figure of merit of the calibration and prediction for the different optical configurations

Conclusions

These first results are very promising for the position F1 and F2 of the multiple fiber probe. However, further improvement is needed in order to achieve a satisfactory accuracy:

- optimization of the distance between emitting and collecting fiber,
- reducing the multiple scattering using several signal preprocessing methods,
- increasing the number of samples in order to increase the robustness of the model.

This "plug and play" optical method offers the potential to be easy to implement to a commercial spectrophotometer and provides the ability to assess sugar content on intact sugar beets. That is a first necessary step for quick in-field assessment, which is, in turn, the main current bottle neck on the varietal selection in breeding programs.