



HAL
open science

Harmonisation of the diagnostic performances of ELISA tests for *C. burnetii* antibodies in ruminants: optimal positivity thresholds and performance reassessment

Laureline Rivière, Elodie Rousset, Elsa Jourdain, Marie Laure Delignette-Muller, T. Lurier

► To cite this version:

Laureline Rivière, Elodie Rousset, Elsa Jourdain, Marie Laure Delignette-Muller, T. Lurier. Harmonisation of the diagnostic performances of ELISA tests for *C. burnetii* antibodies in ruminants: optimal positivity thresholds and performance reassessment. SBED Conference 2024: Insights in Action, Jan 2024, Bruxelles, Belgium. . hal-04513507

HAL Id: hal-04513507

<https://hal.inrae.fr/hal-04513507v1>

Submitted on 20 Mar 2024

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution - NonCommercial - NoDerivatives 4.0 International License

Harmonisation of the diagnostic performances of ELISA tests for *C. burnetii* antibodies in ruminants: optimal positivity thresholds and performance reassessment

Laureline Rivière^{1, 2*}, Elodie Rousset³, Elsa Jourdain¹, Marie-Laure Delignette-Muller², Thibaut Lurier¹

1- UMR INRAE VetAgro Sup EpiA; 2 - UMR CNRS Université Lyon 1 VetAgro Sup 5558; 3 – ANSES Q fever RNL

*corresponding author: laureline.riviere@vetagro-sup.fr

Context

- Several ELISAs are available for the serological diagnosis of *C. burnetii* infection in ruminants.
- **None can be considered as a gold standard** or as a reference test.
- **Differences between their diagnostic performances** (Lurier *et al.* 2021)
 - ⇒ decrease the agreement between the test results from different veterinary laboratories, and
 - ⇒ limits the comparability of surveillance data.
- **Harmonisation** of the tests is possible by **changing their positivity thresholds**.
 - Proposed ROC curves estimation methods (ordered multinomial model – Wang *et al.* 2007 – and mixture model – Choi *et al.* 2006) are not applicable due to the conditional dependency of the tests and to the non-Gaussian distribution of their quantitative measurement.

Objectives

- Identify the positivity thresholds that maximise the agreement between the tests.
- Estimate the impact of changing the thresholds.

Method


- Data: results of three ELISAs from 1258 cattle, 1474 goats and 1432 sheep.
- **Thresholds maximising Hubert's kappa** were identified using a differential evolution algorithm.
- The uncertainty around these optimal thresholds was estimated by bootstrapping.
- **Sensitivities and specificities** of the tests at the optimal thresholds were estimated by **Bayesian inference** using the hierarchical zero-inflated beta-binomial **latent class model** previously described by Lurier *et al.* (2021).

Results

Optimal positivity thresholds

Optimal thresholds are different (higher or lower) from the **manufacturers' thresholds**.

The uncertainty around the optimal thresholds is high, but should be interpreted with caution as the coverage of these bootstrap intervals is not guaranteed in this case.

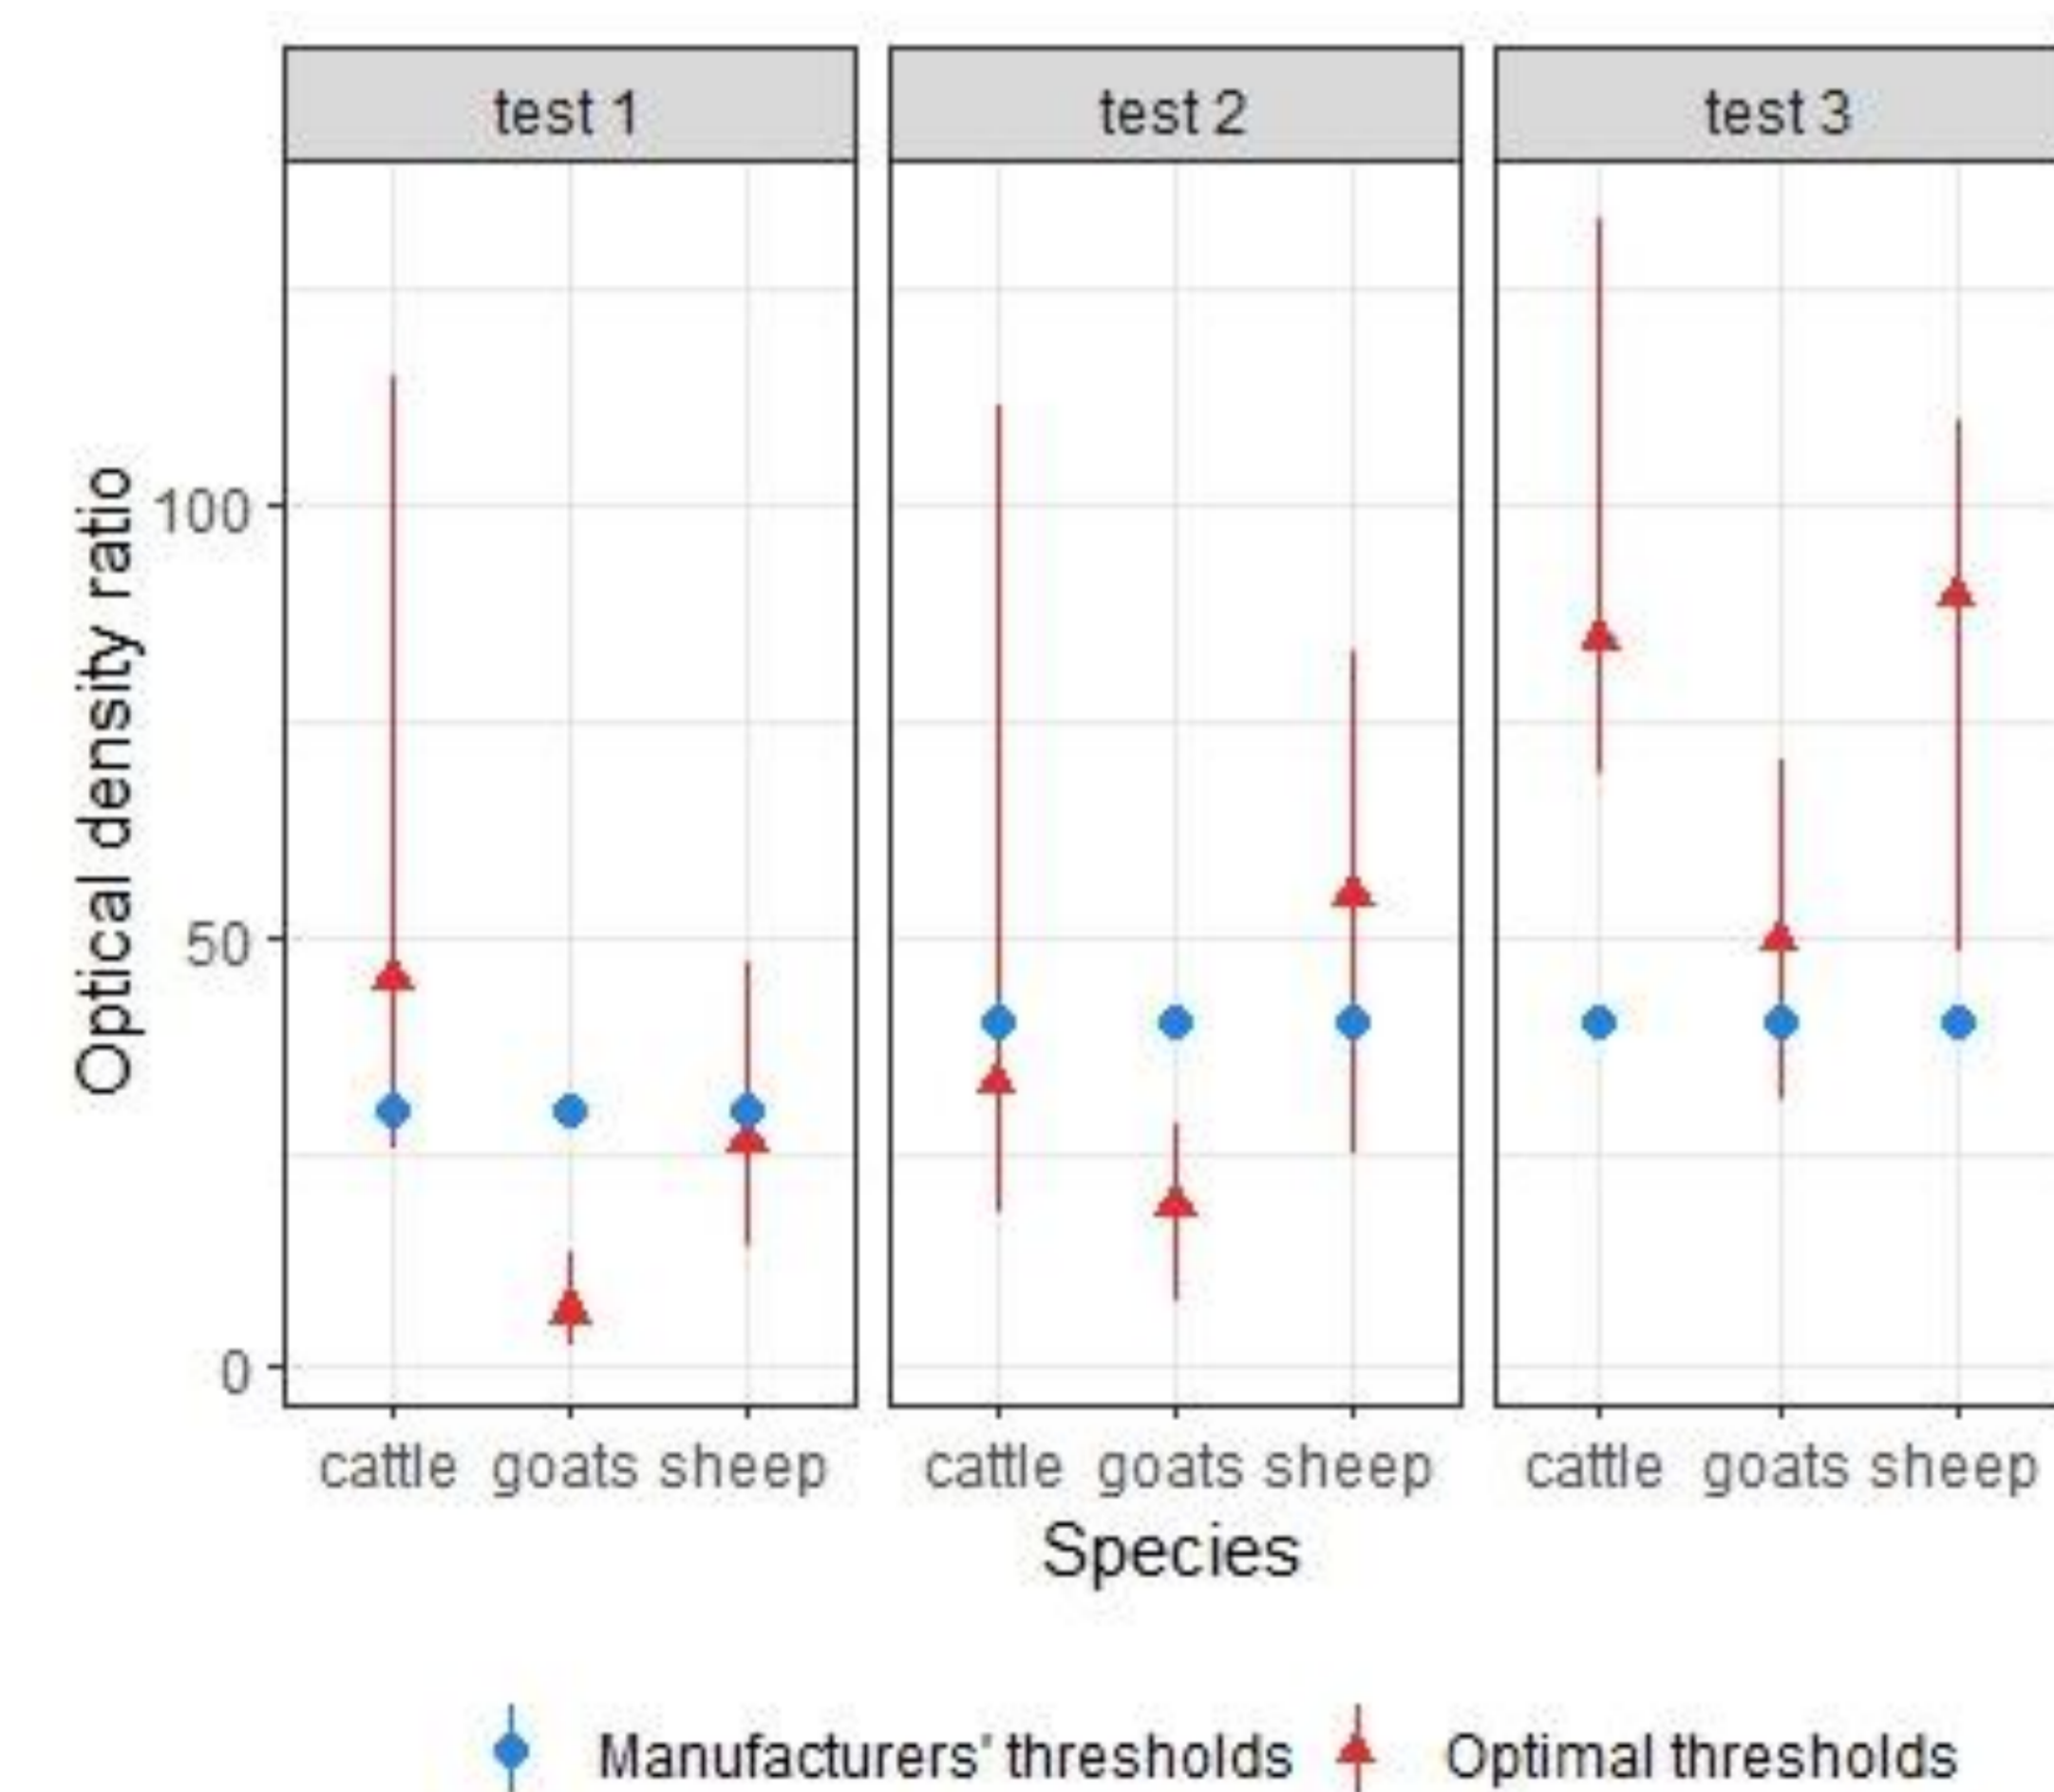


Manufacturers' thresholds and thresholds that maximise Hubert's kappa and their 95% bootstrap intervals

Impact of the threshold change

Diagnostic performances

At the optimal thresholds, the **sensitivities of tests 1 and 2 increased** without major changes in their specificities. The **sensitivity of test 3 decreased** while its **specificity increased**. The sensitivities and specificities are **closer from one test to another**.

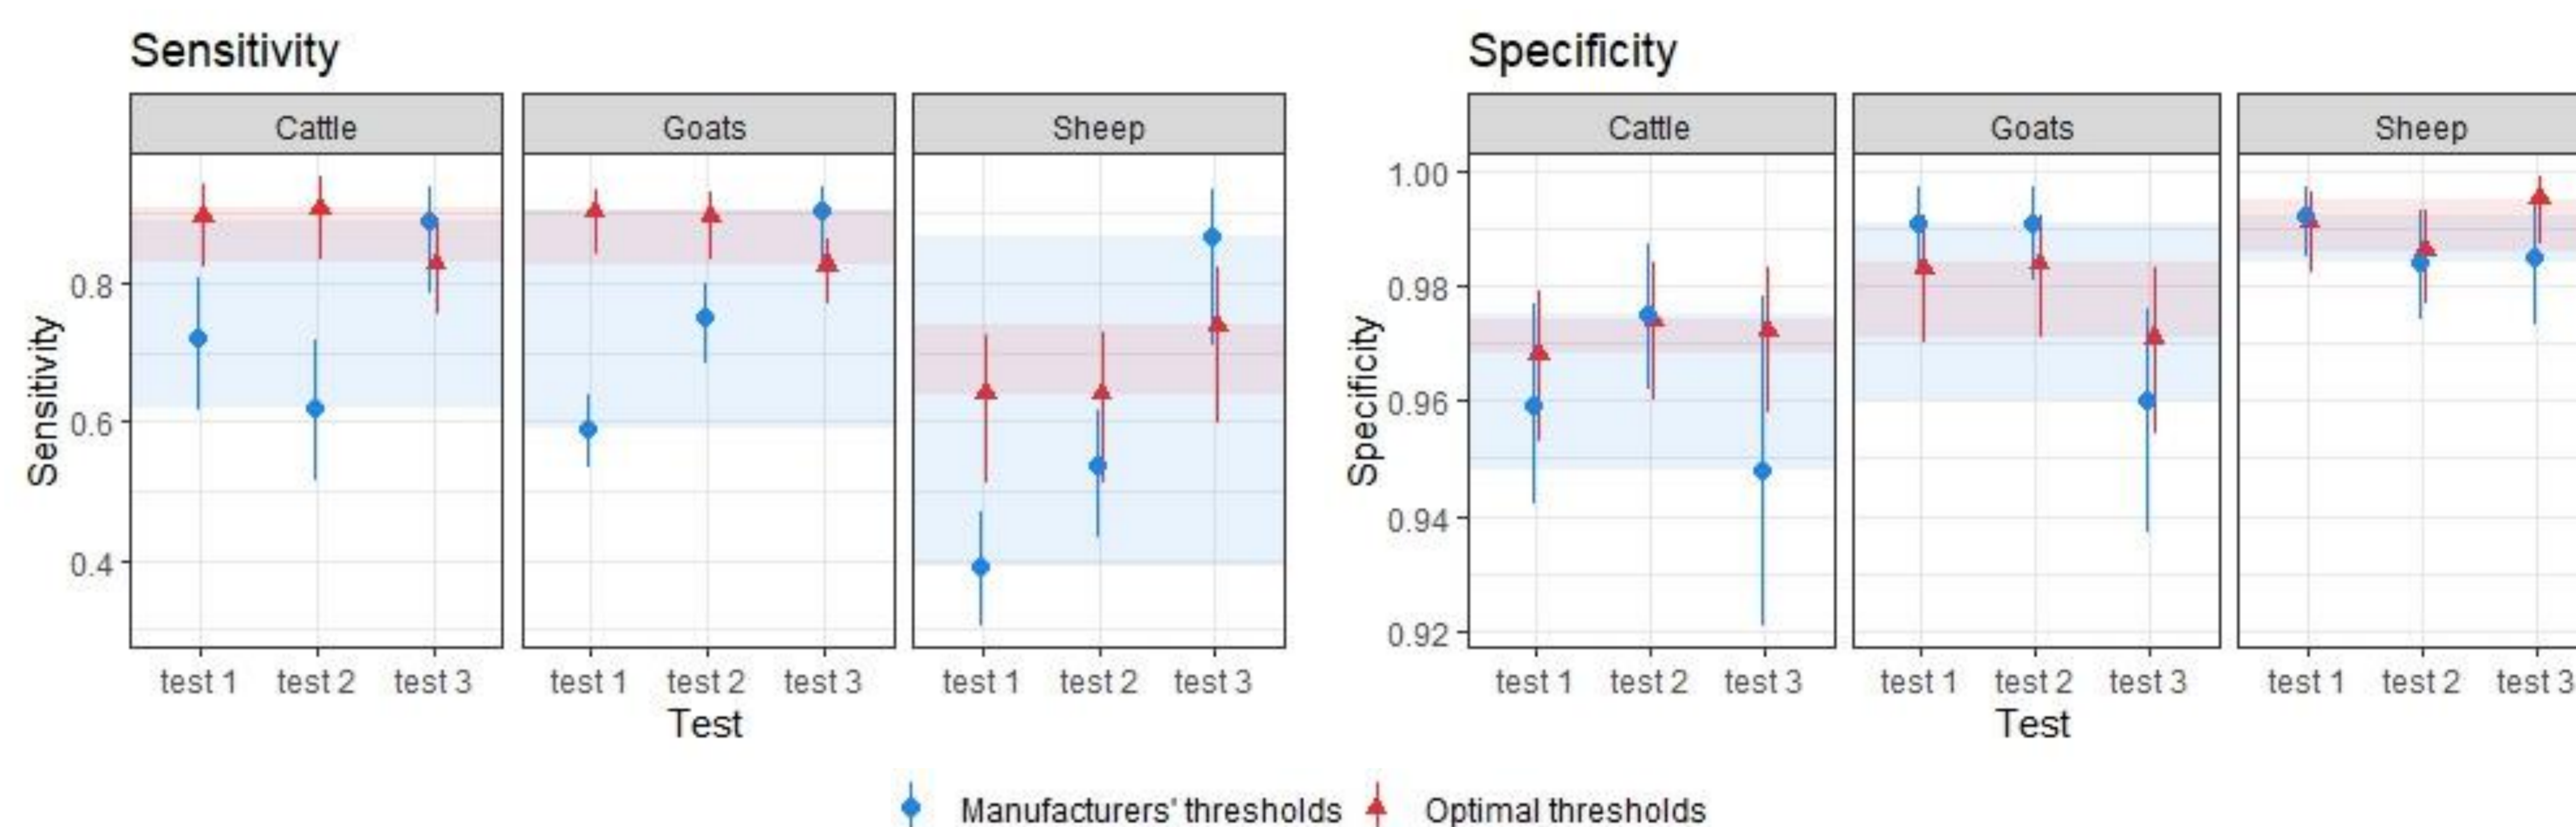

Sensitivity and specificity of the tests at manufacturers' and optimal thresholds and their 95% credibility intervals

Observed disagreement

The proportion of discordant cases is **divided by approximately 2** compared to the manufacturers' thresholds (e.g. from 20 to 12% for goats).

Apparent prevalence

The apparent prevalences are **more similar** from one test to another at the optimal thresholds (e.g. in sheep they range from 7.7 to 17% at the manufacturers' thresholds and from 8.7 to 10.3% at the optimal thresholds).

Findings of the study

Improved harmonisation of the test results and of their diagnostic performances
→ Improved comparability of surveillance data

Discussion and perspective

The increase in sensitivity of tests 1 and 2 estimated in this study is not consistent with the increase in their thresholds compared to the manufacturers' ones.

The development of **methods to evaluate ROC curves in the absence of a gold standard**, especially **considering the conditional dependence** between tests, remains an important area for future research.